

Influence of heart motion on EIT-based stroke volume estimation

Proença M, Braun F, Rapin M, Solà J, Adler A, Grychtol B, Bührer M, Krammer P, Bohm SH, Lemay M, Thiran JP; 15th International Conference on Biomedical Applications of Electrical Impedance Tomography, Gananoque, Ontario, Canada, April 24-26, 2014

Influence of heart motion on EIT-based stroke volume estimation

Martin Proença¹, Fabian Braun^{1,5}, Michael Rapin¹, Josep Solà¹, Andy Adler², Bartłomiej Grychtol³, Martin Bühner⁴, Peter Krammer⁵, Stephan H. Böhm⁵, Mathieu Lemay¹, Jean-Philippe Thiran^{6,7}

¹Systems Division, Swiss Center for Electronics and Microtechnology (CSEM), Neuchâtel, Switzerland, map@csem.ch

²Systems and Computer Engineering, Carleton University, Ottawa, Canada

³Division of Medical Physics in Radiology, German Cancer Research Center (DKFZ), Heidelberg, Germany

⁴Institute for Biomedical Engineering, University and ETH Zurich, Zurich, Switzerland

⁵Swisstom AG, Landquart, Switzerland

⁶Signal Processing Laboratory (LTS5), Swiss Federal Institute of Technology (EPFL), Lausanne, Switzerland

⁷Department of Radiology, University Hospital Center (CHUV) and University of Lausanne (UNIL), Lausanne, Switzerland

Abstract: Cardiac electrical impedance tomography (EIT) signals are affected by myocardial motion. The feasibility of stroke volume estimation using such signals is thus questionable. Results based on a dynamic model show that myocardial motion indeed affects but does not compromise stroke volume estimation.

1 Introduction

In EIT, cardio-synchronous impedance changes in the heart region are assumed to reflect variations of blood volume originating mainly from the ventricles [1]. EIT appears therefore as an interesting continuous and non-invasive modality for monitoring total ventricular volume (TVV), and thus estimating total stroke volume (TSV), defined as the maximal change in TVV over a full cardiac cycle. However, there is increasing evidence that other factors – unrelated to blood volume changes – are contributing to these variations of cardiac-related impedance [2]. In that context, simulations we performed on a finite element 2D extruded dynamic bio-impedance model showed that EIT signals in the heart region might be dominated by myocardial motion-induced changes [3].

These findings raised the question whether heart signals – affected by myocardial motion – remain valid for estimating changes in TVV and thus TSV. The hypothesis that the total impedance change in the heart area remains a true indicator for TVV and TSV is thus investigated here.

2 Methods

To test this hypothesis, we exploited the above 2D dynamic bio-impedance model – created from segmented magnetic resonance (MR) data imaged in the heart horizontal long axis plane – and considered three scenarios: In *Scenario A*, we reproduced cardiac blood volume-related impedance changes by simulating the filling and emptying of the cardiac cavities. In *Scenario B*, myocardial motion-induced changes were reproduced by simulating the dynamics of the heart muscle. Finally, *Scenario C* is the real-case scenario and simulates both blood volume-related and motion-induced changes [3].

These simulations were performed on our finite element model over a full cardiac cycle (corresponding to 20 simulated EIT frames) using the open source EIDORS toolbox, with image reconstruction carried out by the GREIT approach [4]. For each scenario, the impedance change ΔZ – with respect to end-diastole in the heart area – was computed for all frames, thus providing an EIT-based indicator for TVV, according to our hypothesis. Hereafter referred to as TVV_{EIT} , it was expected to

perform best with *Scenario A* (no heart motion) and worse with *Scenario B* (heart motion only).

The reference TVV_{REF} was obtained by summing the volumes V_{LV} and V_{RV} of the left and right ventricles. V_{LV} and V_{RV} were computed via the area-length method [5] – with the areas (Σ_{LV} and Σ_{RV}) and lengths (L_{LV} and L_{RV}) coming from the MR data used to create our model:

$$TVV_{REF} = c_{LV} \cdot \Sigma_{LV}^2 / L_{LV} + c_{RV} \cdot \Sigma_{RV}^2 / L_{RV} \text{ (ml)}, \quad (1)$$

where $c_{LV} = 8/(3\pi)$ [5] and $c_{RV} = 2/3$ [6]. L_{RV} was measured in the vertical long axis plane [6]. The total end-diastolic volume $TEDV_{REF}$ and the total stroke volume TSV_{REF} inferred from TVV_{REF} (see Figure 1) were used to compute TVV_{EIT} by translating ΔZ – normalized by its maximal (systolic) value – into millilitres:

$$TVV_{EIT} = TEDV_{REF} - TSV_{REF} \cdot \Delta Z_{NORM} \text{ (ml)}. \quad (2)$$

3 Results

The estimation error (mean \pm SD) between TVV_{REF} and TVV_{EIT} was of 1.9 ± 13.3 , -14.1 ± 19.5 and -10.1 ± 15.7 ml for *Scenario A*, *B* and *C*, respectively.

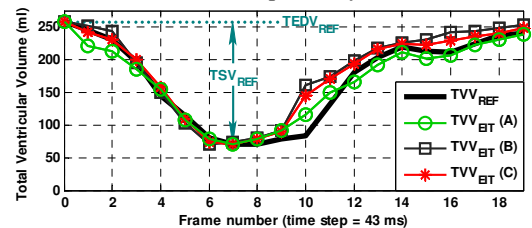



Figure 1: Total ventricular volume estimation using simulated EIT cardiac signals originating from blood volume-related impedance changes (A), motion-induced changes (B), or both (C).

4 Conclusions

In agreement with our expectations, simulations showed that myocardial motion increased the error on TVV_{EIT} and thus EIT-based TSV estimation, without however compromising the approach. When both blood volume changes and myocardial motion are in action (*Scenario C*, real-case scenario) an EIT-based TVV estimation error of -10.1 ± 15.7 ml was obtained, which is sufficiently low to be clinically useful in normal subjects [5].

References

- [1] Eyüboğlu B, et al. *IEEE EMBM* 8:39-45, 1989
- [2] Hellige G, Hahn G. *Critical Care* 15:430, 2011
- [3] Proença M, et al. In *BIOSIGNALS*. 2014 (in press)
- [4] Adler A, et al. *Phys Meas* 30:S35, 2009
- [5] Underwood SR, et al. *Br Heart J* 60:188-195, 1988
- [6] Levine RA, et al. *Circulation* 69:497-505, 1984



Contact us!

call: + 41 (0) 81 330 09 72
mail: info@swisstom.com
visit: www.swisstom.com

Swisstom AG
Schulstrasse 1, CH-7302
Landquart, Switzerland

Swisstom AG

Swisstom AG, located in Landquart, Switzerland, develops and manufactures innovative medical devices. Our new lung function monitor enables life-saving treatments for patients in intensive care and during general anesthesia.

Unlike traditional tomography, Swisstom's bedside imaging is based on non-radiating principles: Electrical Impedance Tomography (EIT). To date, no comparable devices can show such regional organ function continuously and in real-time at the patient's bedside.

Swisstom creates its competitive edge by passionate leadership in non-invasive tomography with the goal to improve individual lives and therapies.