

Assessment of tidal recruitment during inhalation by electrical impedance tomography and dynamic computed tomography -feasibility study in porcine model lavage injury

FPR Toemboel, A Waldmann, S Kampusch, C Bardach, E Kaniusas, S Boehme; European Society of Anaesthesiology (ESA), London, UK, May 28-30, 2016

Assessment of tidal recruitment during inhalation by electrical impedance tomography and dynamic computed tomography - feasibility study in porcine model lavage injury

Toemboel FPR^{1,5}, Waldmann A², Kampusch S^{3,5}, Bardach C^{4,5}, Kaniusas E^{3,5}, Boehme S^{1,5}

¹Medical University of Vienna, Department of Anaesthesia, Pain Management and General Intensive Care Medicine, Vienna, Austria; ²Swisstom AG, Research and Development Department, Landquart, Switzerland; ³Vienna University of Technology, Institute of Electrodynamics, Microwave and Circuit Engineering, Vienna, Austria; ⁴Medical University of Vienna, Department of Biomedical Imaging and Image Guided Therapy, Vienna, Austria; ⁵Vienna EIT Cluster, Austria.

Background and goal of study

Tidal recruitment of atelectasis is a known contributor to ventilator induced lung injury, but its detection remains a challenge.

The most promising technology therefor seems to be electrical impedance tomography (EIT). Our aim was to find a correlate for tidal recruitment by EIT during ongoing respiration compared to dynamic computed tomography (dCT).

Materials and methods

With animal committee approval, 7 mechanically ventilated pigs were studied in healthy and after lung lavage during a pressure ramp maneuver (elisa 800, SALVIA medical, Germany): 0 to 50 mbar (5 mbar/sec).

EIT (PioneerSet, Swisstom, Switzerland) and dCT (Emotion 16, Siemens AG, Germany) were recorded simultaneously and time synchronized. To identify tidal recruitment, we extended the previously described static center of ventilation (CoV) method [1] by computing it dynamically over the inspirational phase (dCoV in EIT). For direct comparison, the center of gravity (dCoG) was post-processed by dCT.

Results and discussion

Both EIT and dCT showed significantly more tidal movement of dCoV and dCoG after lung lavage ($p < .05$, fig.1A). This within-breath shifting towards dependent lung regions during inhalation ($p < .01$, fig.1B) could be attributed to a decrease of atelectatic lung volume as detected by dCT.

The changes in ventilation distribution by tidal recruitment could be followed by the indirect measures of dCoV and dCoG (fig.2) with a high linear correlation (marginal $R^2 = .83$, fig.3).

We performed the measurements during a time-expanded pressure ramp maneuver to capture enough data points with the dCT. The presented dCoV, because of EIT's high temporal resolution, should be appropriate for monitoring tidal recruitment during ongoing tidal ventilation without the need for specific maneuvers.

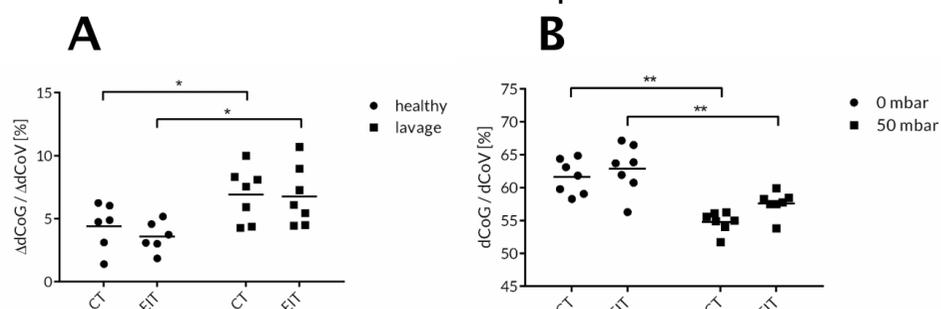


Figure 1. A) Amount of tidal movement of ventilation distribution in dCT and EIT before and after lavage B) dCoG/dCoV at 0 and 50 mbar after lavage. * $p < .05$ ** $p < .01$

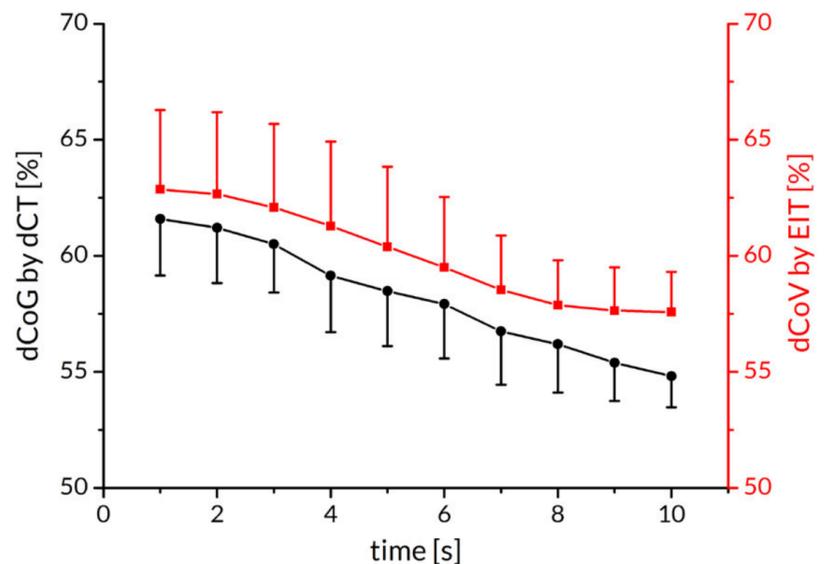


Figure 2. Temporal dynamics of dCoG and dCoV during inhalation after lung lavage.

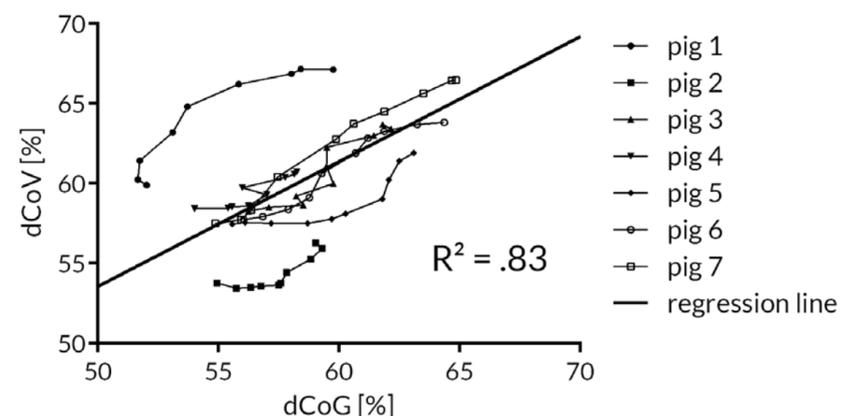


Figure 3. Correlation between dCoG and dCoV after lung lavage

Conclusion


Our data provides first evidence that tidal recruitment can be estimated by the EIT dCoV method.

Acknowledgements

This study is funded by the Vienna Science and Technology Fund (WWTF) through the project LS14-0069. We want to thank all members of the "Vienna EIT Cluster" Markstaller K, Herold C, Thuerk F, Mudrak D, Wielandner A, Prosch H, Jax O, Zbiral M, Gidl D, Weber M, Verdier N.

Reference

1. Frerichs, I., Hahn, G., Golisch, W., Kurpitz, M., Burchardi, H., & Hellige, G. (1998). Monitoring perioperative changes in distribution of pulmonary ventilation by functional electrical impedance tomography. *Acta Anaesthesiologica Scandinavica*, 42(6), 721-6.



Contact us!

call: + 41 (0) 81 330 09 72
mail: info@swisstom.com
visit: www.swisstom.com

Swisstom AG
Schulstrasse 1, CH-7302
Landquart, Switzerland

Swisstom AG

Swisstom AG, located in Landquart, Switzerland, develops and manufactures innovative medical devices. Our new lung function monitor enables life-saving treatments for patients in intensive care and during general anesthesia.

Unlike traditional tomography, Swisstom's bedside imaging is based on non-radiating principles: Electrical Impedance Tomography (EIT). To date, no comparable devices can show such regional organ function continuously and in real-time at the patient's bedside.

Swisstom creates its competitive edge by passionate leadership in non-invasive tomography with the goal to improve individual lives and therapies.